

4(CBA-020-PC

(Dr. dist)

115

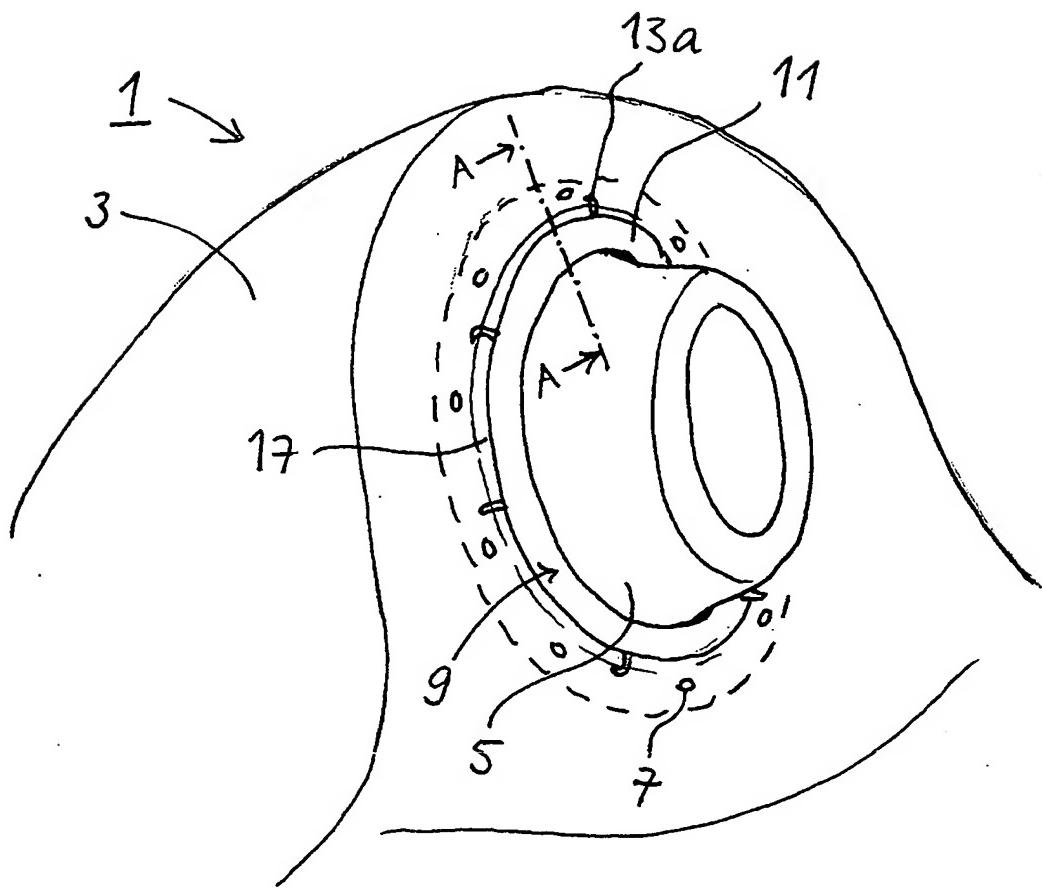


Fig. 1

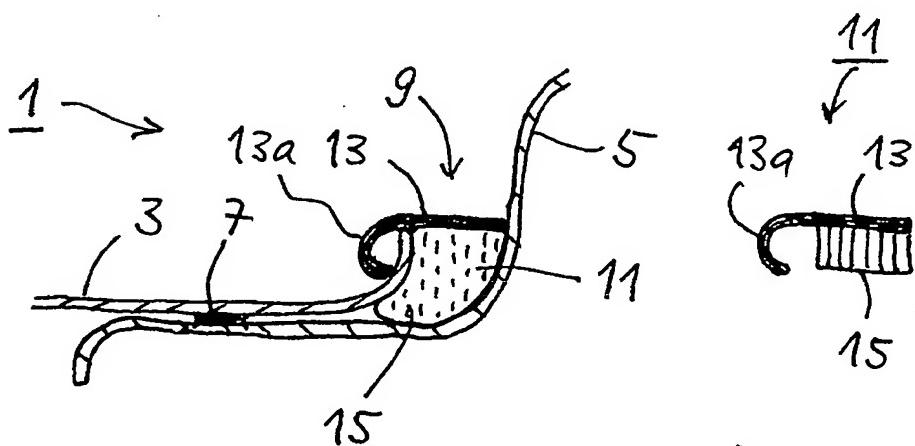


Fig. 2A

Fig. 2B

BEST AVAILABLE COPY

2/5

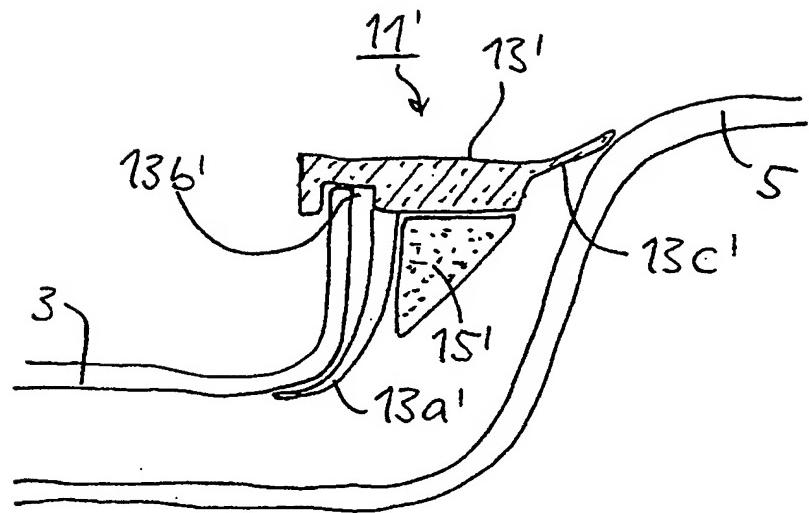


Fig. 3

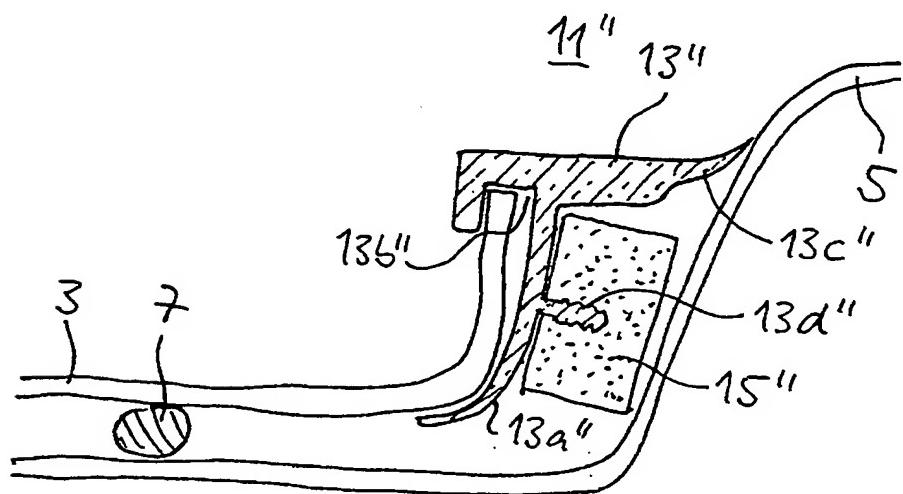


Fig. 4

BEST AVAILABLE COPY

3/5

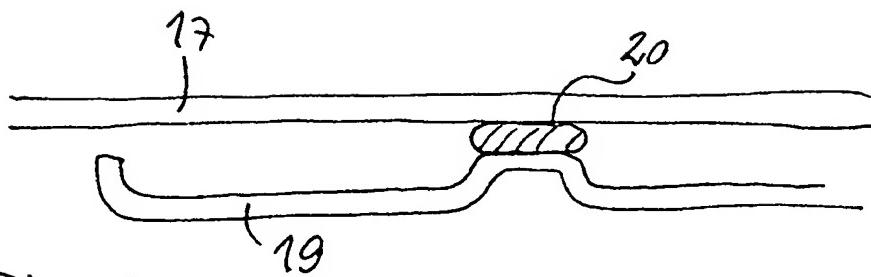


Fig. 5A

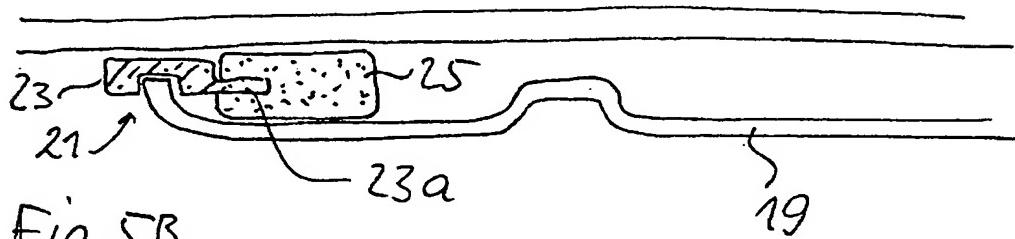


Fig. 5B

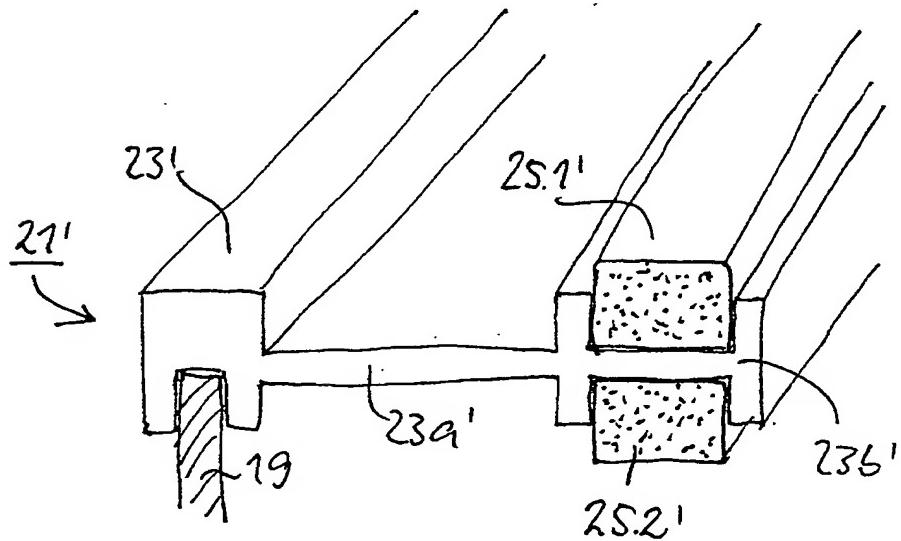


Fig. 6




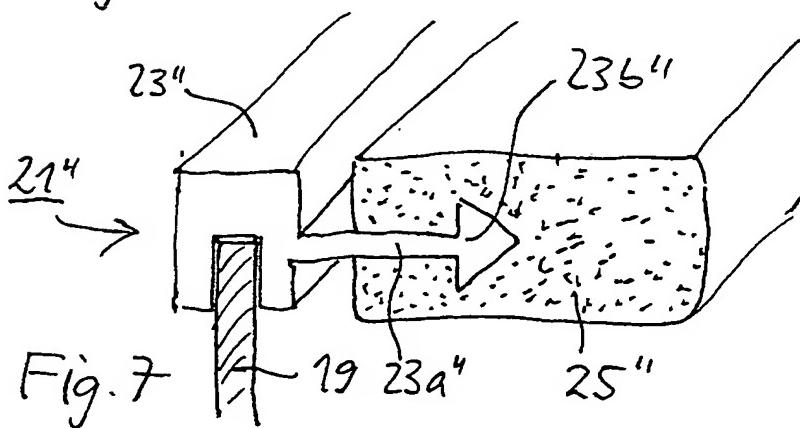


Fig. 7

4/5

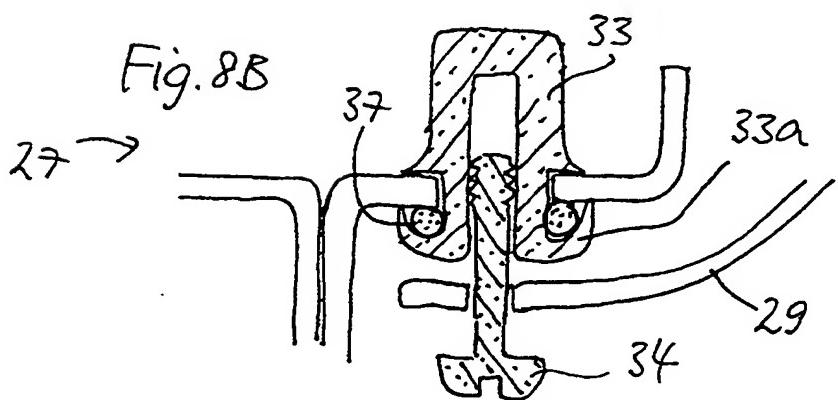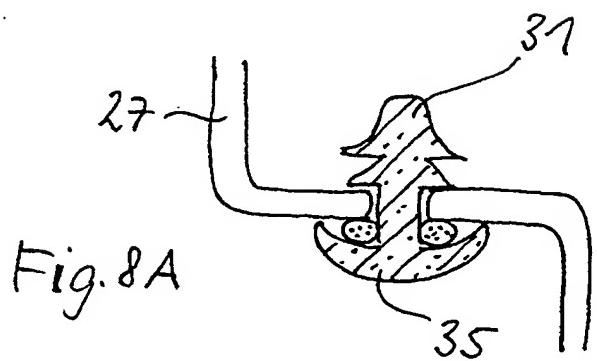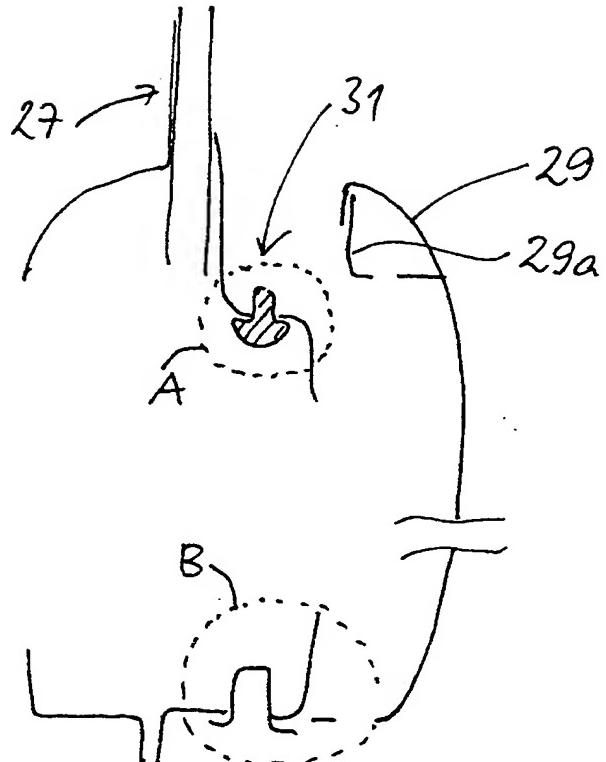

BEST AVAILABLE COPY

5/5

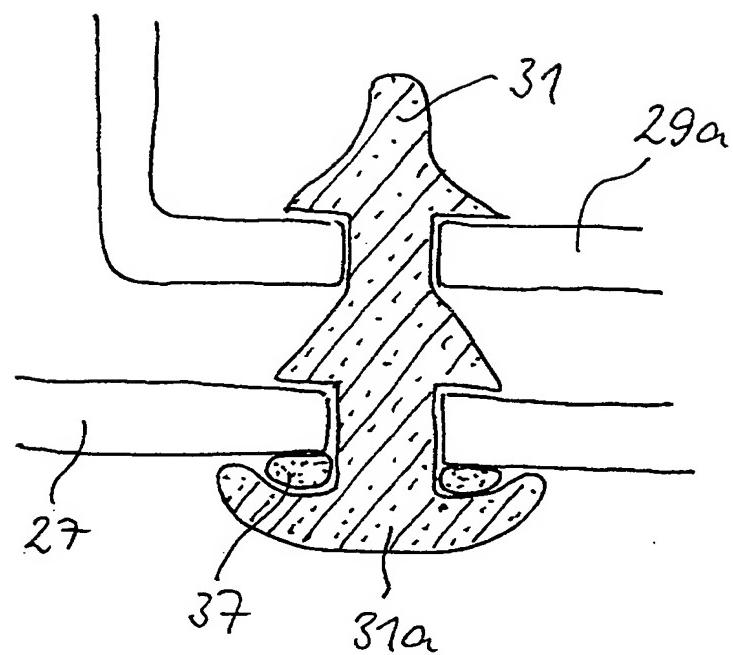


Fig. 8C

BEST AVAILABLE COPY